

HiPer[®] Blood Genomic DNA Extraction Teaching Kit (Magnetic Bead Based) (includes Magnetic stand)

Product Code: HTBM044

Number of experiments that can be performed: 15

Duration of Experiment

Protocol: 1 hour

Agarose Gel Electrophoresis: 1 hour

Storage Instructions:

- The kit is stable for 12 months from the date of manufacture
 - Store Proteinase K at -20°C upon receipt
 - Store 6X Gel Loading Buffer at 2-8 °C
- Other kit contents can be stored at room temperature (15-25°C)

[Index](#)

Sr. No.	Contents	Page No.
1	Aim	3
2	Introduction	3
3	Principle	4
4	Kit Contents	4
5	Materials Required But Not Provided	4
6	Storage	5
7	Important Instructions	5
8	Procedure	5
9	Agarose Gel Electrophoresis	6
10	Quantitation of DNA	6
11	Observation and Result	7
12	Interpretation	7
13	Troubleshooting Guide	8

Aim:

Isolation and purification of genomic DNA from whole blood (using Magnetic bead based).

Introduction:

Blood is a specialized body fluid composed of cells suspended in a liquid called blood plasma. Whole blood contains three types of cells:

1. Red blood cells (RBCs)
2. White blood cells (WBCs)
3. Platelets

Red blood cells (RBCs) do not have any DNA, as they lose their nuclei during maturation. The white blood cell (WBC) component of the blood contains DNA. The blood sample is treated with detergents which break open the cell membrane to release the contents. Enzymes are then used to break down all the proteins, RNA, sugars and fats in the solution.

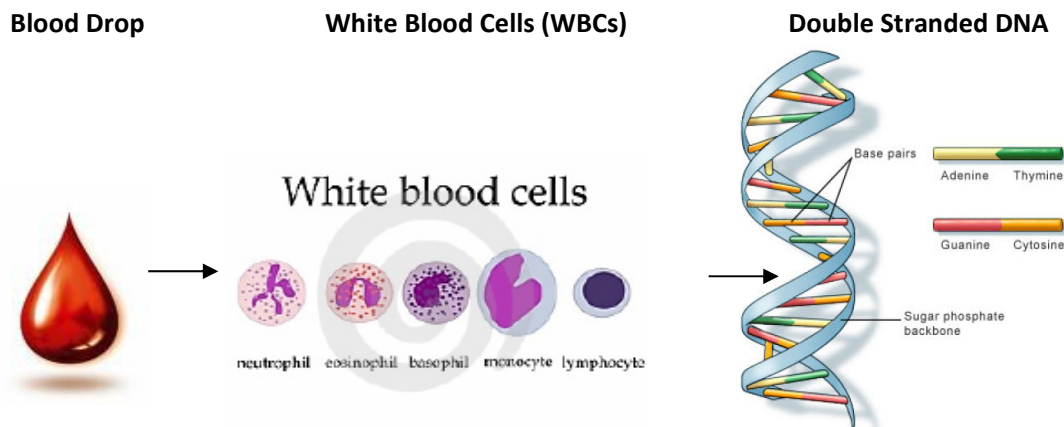


Fig 1: Extraction of blood genomic DNA from white blood cells (WBCs)

Blood Genomic DNA Extraction teaching Kit (Magnetic Bead Based) is designed for rapid extraction and purification of pure genomic DNA from whole blood. It has many advantages over the crude methods of DNA extraction and does not contain harmful organic compounds such as phenol and chloroform.

The DNA purification procedure using the magnetic bead based technology comprises of three steps:

- Adsorption of DNA to the magnetic beads
- Removal of residual contaminants
- Elution of pure genomic DNA

Principle:

HiPer® Blood Genomic DNA Extraction Teaching Kit (Magnetic Bead Based) simplifies the isolation of DNA from fresh blood. Magnetic beads are made up of very small (20 to 30 nm) iron oxide particles, such as particles of magnetite (Fe₃O₄). This gives the beads superparamagnetic properties. Superparamagnetic beads display magnetic behavior only in the presence of an external magnetic field. The small size of the particles enables them to remain separated in suspension, along with whatever they are bound to. Since they don't exhibit magnetic behavior without the presence of a magnetic field, there is no risk of unwanted clumping. Several types of magnetic beads are available based on surface coatings and chemistries. Based on the magnetic beads' binding properties, they can be used for the isolation and purification of DNA, RNA, proteins, and other biomolecules easily and effectively.

Genomic DNA purification from blood involves cell lysis which is achieved by incubation of whole blood in a solution containing chaotropic ions in the presence of Proteinase K at 55°C which helps in the digestion of tissue and cell membranes. After the initial binding of DNA, impurities like proteins, polysaccharides, low molecular weight metabolites and salts are removed by short washing steps. High quality DNA is finally eluted in the Elution Buffer.

Kit Contents:

This kit can be used to extract genomic DNA from whole blood.

Table 1: Enlists the materials provided in this kit with their quantity and recommended storage

Sr. No.	Product Code	Materials Provided	Quantity	Storage
			15 expts	
1	DS0010	Lysis Solution (C1)	8.5 ml	RT
2	ML116	Resuspension Solution (1X PBS)	3.5 ml	RT
3	DS0015	Lysis Solution (AL)	3 ml	RT
4	DS0011	Prewash Solution Concentrate (PW)	4 ml	RT
5	DS0040	Elution Buffer(ET) [10mM Tris-Cl, pH8.5]	1.2 ml	RT
6	DS0013	Proteinase K	0.350 ml	-20 °C
7	DS1005A	Magnetic Beads	0.350 ml	RT
8	DS0003	RNase A (20mg/ml)	0.350 ml	RT
9	MB002	Agarose	7.4 g	RT
10	ML016	50X TAE	180 ml	RT
11	ML015	6X Gel Loading Buffer	0.1 ml	2-8°C
12	LA1109	Magnetic stand	1 No	R T
13	PW147	Collection Tubes, Polypropylene (2.0 ml)	30 No	RT

Materials Required But Not Provided:

Glasswares: Conical flask, Measuring cylinder, Beaker

Reagents: Distilled water, Ethidium bromide (10 mg/ml), Ethanol

Other requirements: Fresh whole blood, Electrophoresis apparatus, Powerpack, UV Transilluminator, Heating block or Water Bath, Vortex Mixer, Tabletop Micro centrifuge (with rotor for 2.0 ml tubes), Micropipettes, Tips, Adhesive tape, Microwave/Burner/Hotplate

Storage:

HiPer® Blood Genomic DNA Extraction Teaching Kit (Magnetic Bead Based) is stable for 12 months from the date of manufacture without showing any reduction in performance. On receipt, store the Proteinase K at -20°C. 6X Gel Loading Buffer should be stored at 2-8 °C. Other kit contents can be stored at room temperature (15-25°C).

Important Instructions:

1. Preheat a water bath or heating block to 55°C.
2. Thoroughly mix the reagents. Examine the reagents for precipitation. If any kit reagent forms a precipitate (other than enzymes), warm at 55-65°C until the precipitate dissolves and allow it to cool down to room temperature (15-25°C) before use.
3. Ensure the use of only clean & dry eppendorf tubes and tips for the procedure.
4. Ensure that the blood is collected under sterile conditions in an anticoagulant coated tube (e.g. EDTA).
5. Ensure that proper/appropriate precautions are taken while handling blood such as wearing nitrile gloves, covering mouth with face mask etc.
6. **Dilution of Prewash Solution Concentrate (PW) – 10ml:** Add 6ml of Ethanol (100%) to 4ml of Prewash Solution Concentrate (PW) to make a final volume of 10ml diluted Wash Solution.

Procedure:

1. Take 200 µl of the fresh whole blood in a 2.0 ml collection tube. Ensure that the blood sample is at room temperature (15-25°C) before beginning the protocol.
2. Add 20 µl of Proteinase K solution into the above collection tube containing blood. Vortex (10-15 seconds) to ensure thorough mixing of the enzyme.
3. Add 20 µl of RNase A solution. Vortex (10-15 seconds) to ensure thorough mixing of the enzyme and incubate for 2 minutes at room temperature.

NOTE: This step helps in getting RNA-free genomic DNA.

4. **Lysis Reaction**
Add 500 µl of Lysis Solution C1 and 20 µl of magnetic beads to the sample, vortex thoroughly for few seconds to obtain a homogenous mixture. Incubate at 55°C for 10 minutes.

NOTE: If cell clumps are visible, pipette the sample gently to obtain a homogenous mixture.

4. Transfer the tubes on Magnetic stand and incubate for 1 minute at Room temperature. Carefully remove and discard the lysate.
6. **First Wash**
Add 600 µl of diluted Wash Solution(2:3) to the beads attached on the wall of collection tube and mix by pipetting .Incubate for 1 minute at Room temperature .

7. Transfer the tubes on Magnetic stand and incubate for 1 minute at Room temperature. Carefully remove and discard the lysate.
8. **Second Wash**
Add 600 μ l of 75% ethanol to the beads attached on the wall of collection tube and mix by pipetting. Incubate for 1 minute at Room temperature.
9. Transfer the tubes on Magnetic stand and incubate for 1 min at Room temperature. Carefully remove and discard the lysate
10. Air dry the tubes for 5 mins at Room temperature
11. **DNA Elution**
Add 100 μ l of Elution Buffer, mix and incubate for 5 minutes at Room Temperature.
12. Transfer the tubes on Magnetic stand and incubate for 1 min at Room temperature , carefully remove and transfer the elute to new 2 ml collection tube.

Agarose Gel Electrophoresis:

Preparation of 1X TAE: To prepare 500 ml of 1X TAE buffer add 10 ml of 50X TAE buffer to 490 ml of sterile distilled water*. Mix well before use.

Preparation of agarose gel: To prepare 50 ml of 0.8% agarose gel, add 0.4 g agarose to 50 ml 1X TAE buffer in a glass beaker or flask. Heat the mixture on a microwave or hot plate or burner by swirling the glass beaker/flask occasionally, until agarose dissolves completely (Ensure that the lid of the flask is loose to avoid buildup of pressure). Allow the solution to cool down to about 55-60°C. Add 0.5 μ l Ethidium bromide, mix well and pour the gel solution into the gel tray. Allow the gel to solidify for about 30 minutes at room temperature.

NOTE: Ethidium bromide is a powerful mutagen and is very toxic. Appropriate safety precautions should be taken by wearing latex gloves; however, use of nitrile gloves is recommended.

Loading of the DNA samples: To prepare sample for electrophoresis, add 2 μ l of 6X gel loading buffer to 10 μ l of DNA sample. Mix well by pipetting and load the sample onto the well. Load the Control DNA after extracting the DNA sample.

Electrophoresis: Connect the power cord to the electrophoretic power supply according to the conventions: Red-Anode and Black- Cathode. Electrophorese at 100-120 volts and 90 mA until dye markers have migrated an appropriate distance, depending on the size of DNA to be visualized.

* Molecular biology grade water is recommended (Product code: ML024).

Quantitation of DNA:

Spectrophotometric analysis and agarose gel electrophoresis will reveal the concentration and the purity of the genomic DNA. Use Elution Buffer to dilute samples and to calibrate the spectrophotometer, measure the absorbance at 260 nm, 280 nm, and 320 nm using a quartz microcuvette. Absorbance readings at 260 nm should fall between 0.1 and 1.0. The 320 nm absorbance is used to correct

background absorbance. Purity is determined by calculating the ratio of absorbance at 260 nm to absorbance at 280 nm. The concentration of DNA is calculated by the following formula:
 Concentration of DNA sample ($\mu\text{g/ml}$) = $200 \times A_{260} \times \text{dilution factor}$

Observation and Result:

Perform Agarose Gel Electrophoresis. Visualize the DNA bands using UV transilluminator and calculate the yield and purity using UV Spectrophotometer.

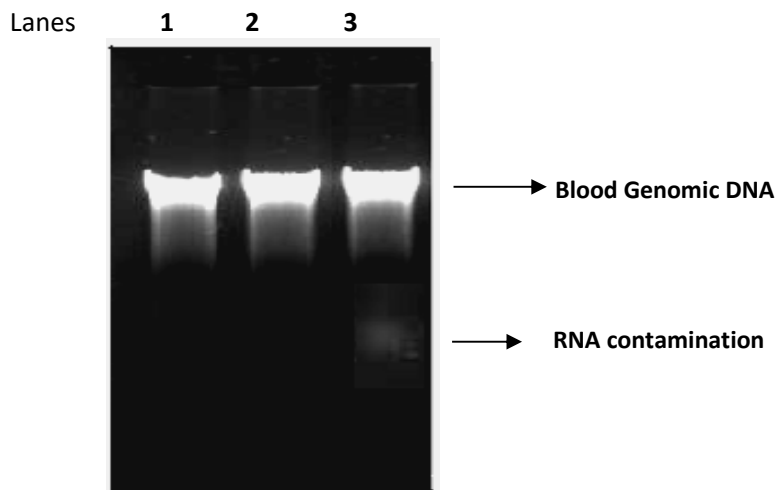


Fig 2: Gel image of isolated blood genomic DNA

Lane 1 and 2: Blood Genomic DNA

Lane 3: Blood Genomic DNA with RNA contamination

Table 2: Absorbance of the extracted genomic DNA at 260 nm and 280 nm

Sample	Dilution Factor	A_{260}	A_{280}	A_{260}/A_{280}	Concentration ($\mu\text{g/ml}$)
1					
2					
3					

Calculate the concentration of isolated DNA using following formula:

Concentration of DNA sample ($\mu\text{g/ml}$) = $200 \times A_{260} \times \text{dilution factor}$

Interpretation:

The lanes 1 and 2 demonstrate that highly purified blood genomic DNA has been obtained with no visible RNA contamination when electrophoresed on agarose gel. If RNA contamination is present, one

would see a faint and smeary RNA band below the genomic DNA as shown in lane 3 since RNA being of lower molecular weight than DNA runs faster than the genomic DNA. RNA contamination is observed when the RNase treatment has either been skipped or not been carried out properly.


An absorbance of 1.0 at 260 nm corresponds to approximately 50 µg/ml of DNA. If the A_{260}/A_{280} ratio is 1.6-1.9, then the isolated DNA sample is considered to be pure. If higher A_{260}/A_{280} ratio is observed it indicates the possibility of RNA contamination.

Troubleshooting Guide:

Sr. No.	Problem	Possible Cause	Solution
1	Presence of cell clumps/colored residue on the spin column after washing	Inefficient cell lysis due to improper mixing of the Lysis Solution with the blood sample	The sample and the Lysis Solution should be mixed thoroughly by pulse-vortexing
		Due to decreased Proteinase K activity	Do not add Proteinase K directly to the Lysis Solution
2	Poor or low genomic DNA recovery	DNA elution is improper	Ensure that DNA elution is in 200 µl of Elution Buffer. To improve the DNA yield, incubate for 5 minutes at room temperature after the addition of Elution Buffer
3	Shearing of genomic DNA	The blood sample used is old, degraded	If the blood sample is old the eluate may yield degraded DNA. For best results fresh whole blood should be used

Technical Assistance:

At HiMedia we pride ourselves on the quality and availability of our technical support. For any kind of technical assistance, mail at mb@himedialabs.com



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Private Limited,
Reg. Off: Plot No. C-40, Road No. 21Y,
MIDC, Wagle Industrial Area, Thane,
(West) 400604, Maharashtra, INDIA.
Web: www.himedialabs.com



10/2025

PIHTBM044_O/1022

HTBM044-00

Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal or therapeutic use but for laboratory, diagnostic, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

HiMedia Laboratories Pvt. Ltd. Reg. office : Plot No. C-40, Road No. 21Y, MIDC, Wagle Industrial Area, Thane, (West) 400604, Maharashtra, INDIA.
Customer Care No.: 00-91-22-6116 9797 Tel: 00-91-22-6147 1919, 6903 4800 Email: techhelp@himedialabs.com Website: www.himedialabs.com