

## MBPCR088

## Hi-PCR<sup>®</sup> 18S rRNA SYBr PCR Kit

### Description:

Eukaryotic 18S ribosomal RNA (rRNA) gene primers that feature a wide coverage are critical in detecting the composition of eukaryotic microscopic organisms in ecosystems. Here, 18S rRNA primers based on consecutive conserved sites and evaluated their coverage efficiency and scope of application to different eukaryotic groups. Common conserved regions in eukaryotic 18S rRNA sequences is used to design 18S universal primers.

Real-time PCR detection is an important molecular method for diagnosis that amplifies and accurately identifies 18S rRNA specific nucleic acid for diagnosis in clinical samples. PCR assays offer several features that could overcome current shortcomings for the diagnosis of clinical samples

The Hi-PCR<sup>®</sup> 18S rRNA SYBr PCR Kit is designed to specifically amplify a region (approx. 182bp) within the 18S rRNA.

**NOTE: The Hi-PCR<sup>®</sup> 18S rRNA SYBr PCR Kit is for *in vitro* use only.**

### Principle:


The Hi-PCR<sup>®</sup> 18S rRNA SYBr PCR Kit is designed for the detection of a specific sequence of the **18S rRNA gene** in food, clinical samples, environmental samples etc. The 18S rRNA specific primers generate an amplicon of **182 bp**. This kit also contains **Positive control**.

**Positive control:** This is a control reaction using a known template. A positive control is usually used to check that the primers have been designed properly and the PCR conditions have been set up correctly.





Real-time Polymerase Chain Reaction, also called quantitative Polymerase Chain Reaction (qPCR) or kinetic Polymerase Chain Reaction, is a laboratory technique based on the principle of Polymerase Chain Reaction. This technique is used to amplify and simultaneously quantitate a targeted DNA sequence. Real-time PCR systems based on SYBr Green assays have increasingly been used for accurate, reliable detection and quantitation of various food-borne pathogens. HiMedia's Hi-PCR<sup>®</sup> 18S rRNA SYBr PCR Kit is one such SYBr green based qPCR technique which allows amplification of **18S rRNA gene**.

**Diagrammatic representation of preferential binding of SYBr Green Dye to specific DNA fragments in real-time PCR.**

- a) Dye in solution emits low fluorescence      b) Emission of the fluorescence by binding      c) Amplification data



**SYBr Green dye cycles between an unbound (Denaturation step) and a bound (Annealing through Extension) state as the reaction progresses. Signal intensity increases as the quantity of amplicons increase in later cycles indicating amplification. During elongation, more and more dye molecules bind to the newly synthesized DNA. If the reaction is monitored continuously, an increase in fluorescence is viewed in real-time. Upon denaturation of the DNA for the next heating cycle, the dye molecules are released and the fluorescence signal falls.**

Keys : SYBr   
 Forward primer   
 Reverse primer   
 DNA Strand 

**Features:**

- Fast and simple
- Sensitive and specific results
- Guaranteed reproducible results

**Sample Source:** Food, clinical and environmental samples

**Storage:**

The provided kit has a shelf-life of 12 months when stored between -10°C to -20°C. Repeated thawing and freezing of PCR reagents should be avoided, as this may reduce the sensitivity. If reagents are to be used multiple times, we recommend storing reagents as aliquots to avoid repeated freeze and thaw. Degradation of sample DNA specimens can also reduce sensitivity of the assay. HiMedia does not recommend using the kit after the expiry date stated on pack.

**Kit Contents:**

The provided PCR kit contains:

Components	Product code	Reagents provided for (reactions)*( $\mu\text{L}$ )	
		25R	50R
Hi-SYBr Master Mix (with Taq Polymerase)	MBT074	338	675
18S Primer mix	DS0300	27	54
Positive control DNA	DS0122B	5	10
Molecular Biology Grade Water for PCR	ML065	300	600

\* For a 20 $\mu\text{L}$  PCR reaction

**Specimen collection and Handling**

Follow appropriate techniques for handling specimens; after use, contaminated materials must be sterilized by autoclaving before discarding. Standard precautions as per established guidelines should be followed while handling clinical specimens and items contaminated with blood and other body fluids. Safety guidelines may be referred in individual safety data sheets.

**Sample Preparation:**

Various food, clinical and environmental samples are routinely examined. For extraction and purification of high yield and pure DNA, perform the nucleic acid purification using HiMedia's Extraction kits.

**Materials needed but not provided:**

- PCR tubes (Product code PW1255) or PCR Strips (Product code: PR17) or PCR Plates (Product code: PR2 / PR3 / PR19) & Sealing film (PR18)
- Insta Q Real Time PCR System (Product Code: LA1012/LA1073/LA1023/LA1024/LA1074)
- Barrier Micropipette Tips (Product Code: LA749 / LA749A / LA751 / LA751A / LA750 / LA750A / LA859 / LA859A)
- Micropipettes

**General Preparation Instructions:**

- Before use all PCR components should be completely thawed on ice (4°C).
- Perform the amplification reactions in a clean area, preferably in a biosafety cabinet.
- Use of aerosol barrier pipette tips is recommended to reduce contamination risks from extraneous DNA templates.
- Extract and store positive control sample (if used) separately from all other reagents to avoid contamination and add it to the reaction mix in a separate area.

**A. Protocol for PCR Master Mix Preparation**

Perform PCR reactions for each DNA sample as per the following table:

Components	Product Code	Recommended volume to be added per reaction ( $\mu\text{L}$ )
Hi-SYBr Master Mix (with Taq Polymerase)	MBT074	12.5 $\mu\text{L}$
18S Primer mix	DS0300	1 $\mu\text{L}$
Template DNA	-	1-2 $\mu\text{L}$
Molecular Biology Grade Water for PCR	ML065	Up to 25 $\mu\text{L}$

**NOTE: (Optional) – The user can also set up an additional PCR reaction containing 1 $\mu\text{L}$  of Positive control DNA (DS0122B) (provided) in a separate tube.**

Centrifuge the tube briefly at 6000 rpm for about 10 seconds. Place the tubes in real-time PCR machine and set the recommended PCR program (mentioned below). Interpret the data from the amplification plot (observe the Ct values).

**B. Recommended PCR program**

- 1. Initial denaturation : 94°C for 5 minutes No. of cycles: 1
- 2. Denaturation : 94°C for 45 seconds
- 3. Annealing (Plate Read) : 58°C for 30 seconds } No. of cycles: 40
- 4. Melt Curve Analysis as per HiMedia’s Insta Q96 Real-Time PCR Machine
  - 95°C : 15 seconds
  - 60°C : 1 minute
  - 95°C : 15 seconds
  - Increment : 0.5°C
  - On Hold : 10 seconds
- 5. Hold : 4°C for ∞


**NOTE: The user can also set up a melt curve program as per their existing PCR instrument.**

**Quality Control**


Each lot of HiMedia’s Hi-PCR® 18S rRNA SYBr PCR Kit is assayed for contaminating endonuclease, exonuclease and non-specific DNase activities. Functionally tested in DNA amplification.

**Amplification Data:**

**Amplification plot**

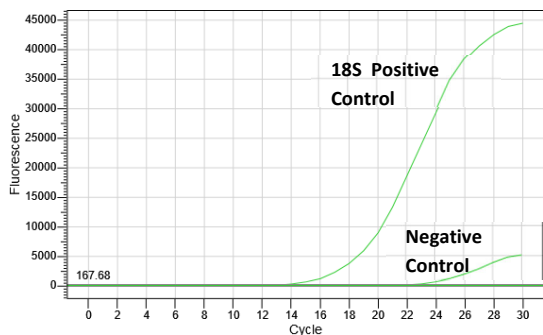

**Melt curve**

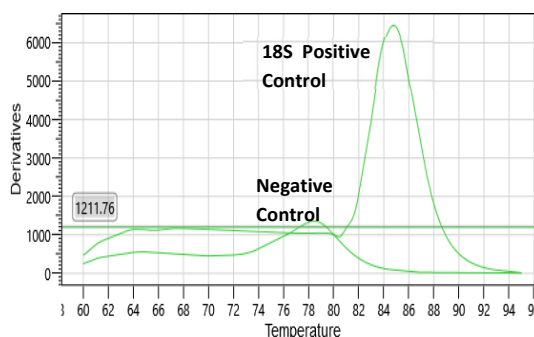

Sr. No.	Sample	C <sub>t</sub> value	T <sub>m</sub> (°C)
1	Positive control	13.2	84.8
2	Negative control	21.8	78.5

Figure: Data representing real-time amplification data of 18S rRNA PCR with C<sub>t</sub> values (provided in table)

**Data Interpretation**

Melting Temperature (T <sub>m</sub> )*	Result Interpretation
84°C-86°C	Positive for 18S

\* T<sub>m</sub> values can slightly vary for different sample types. If the T<sub>m</sub> values show significant variation from those mentioned in the above table, then the sample is considered to be negative for 18S gene.

### Troubleshooting Guide:

Sr.No.	Problem	Cause	Solution
1.	No amplification	Degraded samples	1. Check the integrity of DNA using agarose gel electrophoresis. 2. Use freshly prepared DNA to ensure the availability of intact template sequence for efficient amplification.
		Error in protocol setup	Verify that the correct reagent volumes, dilutions and storage conditions have been used.
2.	Variability between replicates	Error in reaction set-up	Prepare large volume master mix, vortex thoroughly and aliquot into reaction tubes.
		Air bubbles in reaction mix	Briefly centrifuge reaction samples/plate prior to running on a real-time PCR instrument.
		Pipetting error	C <sub>t</sub> values of replicates can show increased variation due to poor laboratory technique or imprecise pipettes.
3.	Amplification in negative control	Reagents contaminated	1. Replace all critical solutions 2. Repeat the analysis of all tests with fresh aliquots of critical reagents.

### Safety Information


The Hi-PCR® 18S rRNA SYBr PCR Kit is for laboratory use only, not for drug, household or other uses. Take appropriate laboratory safety measures and wear gloves when handling.

### Disposal

User must ensure safe disposal by autoclaving and/or incineration of used or unusable preparations of this product. Follow established laboratory procedures in disposing of infectious materials and material that comes into contact with clinical sample must be decontaminated and disposed off in accordance with current laboratory techniques.

### Technical Assistance

At HiMedia, we pride ourselves on the quality and availability of our technical support. For any kind of technical assistance, mail at [mb@himedialabs.com](mailto:mb@himedialabs.com).



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Private Limited,  
Reg. Off: Plot No. C-40, Road No. 21Y,  
MIDC, Wagle Industrial Estate, Thane,  
(West) 400604, Maharashtra, INDIA.  
Web: [www.himedialabs.com](http://www.himedialabs.com)



03/2027

PIMBPCR088\_O/0324

MBPCR088-05

**Disclaimer :**

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal or therapeutic use but for laboratory, diagnostic, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

HiMedia Laboratories Pvt. Ltd. Reg.office : Plot No. C-40, Road No. 21Y, MIDC, Wagle Industrial Estate, Thane, (West) 400604, Maharashtra, INDIA. Customer Care No.: 00-91-22-6116 9797 Tel: 00-91-22-6147 1919, 6903 4800 Email: [mb@himedialabs.com](mailto:mb@himedialabs.com) Website: [www.himedialabs.com](http://www.himedialabs.com)