

## MBPCR168

## Hi-PCR® Peste des petits ruminants (PPR) Probe PCR Kit

### Description

Peste des petits ruminants (PPR) are an acute or subacute viral disease of goats and sheep characterized by fever, necrotic stomatitis, gastroenteritis, pneumonia and sometimes death. The causal virus, a member of the Morbillivirus genus in the family Paramyxoviridae, preferentially replicates in lymphoid tissues and epithelial tissue of the GI and respiratory tracts, where it produces characteristic lesions. The genus Morbillivirus from the family Paramyxoviridae, a group of enveloped viruses with non-segmented, negative-strand RNA genomes is a virus that is highly infectious, spreads via the respiratory route and causes profound immune suppression. With animal healthcare becoming increasingly important, specific and faster methods for pathogen detection are the need of the hour.

**NOTE:** HiMedia's Hi-PCR® Peste des petits ruminants (PPR) Probe PCR Kit is for *in-vitro* use only.

### Intended Use

Recommended for sensitive and specific detection of PPR in animal samples.

### Principle

Real-time polymerase chain reaction, also called quantitative Polymerase Chain Reaction (qPCR) or kinetic Polymerase Chain Reaction, is a laboratory technique based on the principle of PCR. This technique is used to amplify a targeted DNA sequence by use of hydrolysis probes that are short oligonucleotides that have a fluorescent reporter dye attached to the 5' end and a quencher dye to the 3' end. HiMedia's Hi-PCR® Peste des petits ruminants (PPR) Probe PCR Kit is designed to detect the **PPRV specific gene in FAM channel and Internal Control in JOE channel**. The kit allows rapid, sensitive and specific detection of PPR. This kit also contains Positive control.

### Negative Control

A negative control is needed to ensure that the reagents, equipment, and environment used in the assay is not contaminated. In this reaction, nuclease free water is used as the template.


### Positive control

This is a control reaction using a known template (target pathogen). A positive control is usually used to check that the primers have been designed properly and the PCR conditions have been set up correctly.

### Internal Control

This is a control sequence which is amplified in the same reaction tube along with the target sequence (target species) but detected with a different primer (i.e. Multiplex PCR). An internal control is often used to detect the failure of amplification in cases where the target sequence is not amplified.

## Diagrammatic representation of preferential binding of probe specific to DNA fragments in Real-time PCR

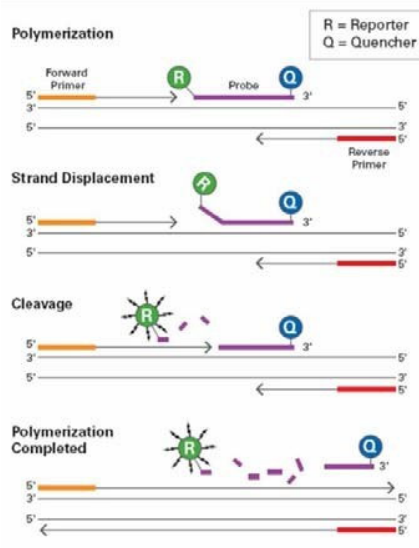

**Polymerization:** A fluorescent reporter (R) dye and a quencher (Q) are attached to the 5' and 3' end of the probe respectively

**Strand displacement:** When the probe is intact, the report dye emission is quenched.

**Cleavage:** During each extension cycle, the DNA polymerase cleaves the reporter dye from the probe

**Polymerization completed:** Once separated from the quencher, the reporter dye emits its characteristic fluorescence

While the probe is intact, the proximity of the quencher dye greatly reduces the fluorescence emitted by the reporter dye by fluorescence resonance energy transfer (FRET). The probes are designed such that they anneal within a DNA region amplified by a specific set of primers. During PCR amplification, these probes will hybridize to the target sequences located in the amplicon i.e. the DNA. As the *Taq* DNA polymerase replicates the template with the bound probe, the 5'-nuclease activity of the polymerase enzyme cleaves the fluorescent probe. The end result in cleavage of the probe is separation of the reporter dye from the quencher dye and increasing the reporter dye signal. As the probe is removed from the target strand, primer extension continues to the end of the template strand. Hence, fluorescence detected in the quantitative PCR thermal cycle is directly proportional to the fluorophore released and the amount of DNA template present in the PCR. Thus, inclusion of the probe does not inhibit the overall PCR process.

### Features

- Fast and simple
- Good sensitivity and specific results
- Guaranteed reproducible results
- Rapid detection of all relevant clinical pathogens

**Sample Source:** Whole Blood, Swabs from conjunctival discharges or nasal buccal or rectal mucosae, necropsy samples from lymph nodes, bronchial nodes, lungs, spleen.

### Specimen collection and Handling

Follow appropriate techniques for handling specimens; after use, contaminated materials must be sterilized by autoclaving before discarding. Standard precautions as per established guidelines should be followed while handling clinical specimens and items contaminated with blood and other body fluids. Safety guidelines may be referred in individual safety data sheets.

### Storage and Shelf life

The provided kit has a shelf-life of 12 months when stored at  $-20^{\circ}\text{C}$ . Repeated thawing and freezing of PCR reagents should be avoided, as this may reduce the sensitivity. If the reagents are to be used multiple times, we recommend storing reagents as aliquots to avoid repeated freeze and thaw. Degradation of sample DNA specimens can also reduce the sensitivity of the assay. HiMedia Laboratories does not recommend using the kit after the expiry date stated on pack.

**Kit Contents:** The provided PCR kit contains

Components	Product code	Reagents provided for (reactions)* (µL)	
		25R	50R
2X One step buffer mix	DS1086	338	675
One -step RT enzyme mix	DS1087	22	43.2
PPR Primer-Probe Mix	DS0557	27	54
Internal Control Primer-Probe Mix	DS1021	27	54
Internal Control DNA	DS1022C	27	54
PPR Positive Control	DS0271	25	50
Molecular Biology Grade Water for PCR	ML065	150	300

\* For a 25 µL PCR reaction

**Materials needed but not provided:**

- PCR tubes (Product code PW1255) or PCR Strips (Product code: PR17) or PCR Plates (Product code: PR2 / PR3 / PR19) & Sealing film (PR18)
- Insta Q Real Time PCR System (Product Code: LA1012 / LA1023 / LA1024 / LA1073)
- Barrier Micropipette Tips
- Micropipettes
- HiPurA® Viral RNA Purification Kit (MB615)

**General Preparation Instructions**

- Before use all PCR components should be completely thawed on ice (4°C).
- Perform the amplification reactions in a clean area, preferably in a biosafety cabinet.
- Use of aerosol barrier pipette tips is recommended to reduce contamination risks from extraneous DNA templates.
- Extract and store positive control sample (if used) separately from all other reagents to avoid contamination and add it to the reaction mix in a separate area.

**A. Protocol for PCR Master Mix Preparation**

Components	Product code	Volume to be added for 1R (for a 25 µL reaction)
2X One step buffer mix	DS1086	12.5
One -step RT enzyme mix	DS1087	0.8
PPR Primer-Probe Mix	DS0557	1.0
Internal Control Primer-Probe Mix	DS1021	1.0
Internal Control DNA	DS1022C	1.0
Test – Extracted Sample RNA Positive Control – Provided in Kit Negative Control - Water	-	5.0
Molecular Biology Grade Water for PCR	ML065	3.7
<b>Total volume</b>	-	<b>25</b>

Centrifuge the tube briefly at 6000 rpm for about 10 seconds. Place the tubes in Real-time PCR machine and set the recommended PCR program (mentioned below). Interpret the data from the amplification plot (observe the Ct values).

**B. Recommended PCR program**

- |                          |                       |                     |
|--------------------------|-----------------------|---------------------|
| 1. Reverse Transcription | : 50°C for 15 minutes |                     |
| 2. Initial denaturation  | : 95°C for 03 minutes |                     |
| 3. Denaturation          | : 95°C for 15 seconds | } No. of cycles: 40 |
| 4. Annealing             | : 55°C for 30 seconds |                     |
| 5. Plate Read            | : FAM/JOE             |                     |
| 6. Hold                  | : 4°C for ∞           |                     |

#for instruments not calibrated for JOE, HEX can be used

**Warning and Precautions**

Not for Medicinal Use. Read the procedure carefully before beginning the protocol. Wear protective gloves/protective clothing/eye protection/face protection. Follow good clinical laboratory practices while handling clinical samples. Standard precautions should be followed as per established guidelines. Safety guidelines may be referred in safety data sheets of the product.

**Limitations**

Although rare, mutations within the highly conserved regions of the targets genes covered by the kit’s primers and/or probe may result in under quantitation or failure to detect the presence of the target regions in these cases. Validity and performance of the assay design are revised at regular intervals.

**Performance and Evaluation**

Each lot of HI Media’s Hi-PCR® Peste des petits ruminants (PPR) Probe PCR Kit is tested against predetermined specifications to ensure consistent product quality.

**Quality Control**

Each lot of HI Media’s Hi-PCR® Peste des petits ruminants (PPR) Probe PCR Kit is assayed for contaminating endonuclease, exonuclease and non-specific DNase activities. Functionally tested in RNA amplification.


**Data Analysis**

The following conditions should be met for a valid diagnostic test:

Control	Detection channel	
	FAM (PPR)	JOE (Internal Control)
Positive Control	+	+/-*
Negative Control	-	+

\*The presence or absence of a signal in the JOE channel is not relevant for the validity of the test run due to competition between the test template and Internal Control template.

**Amplification Data**

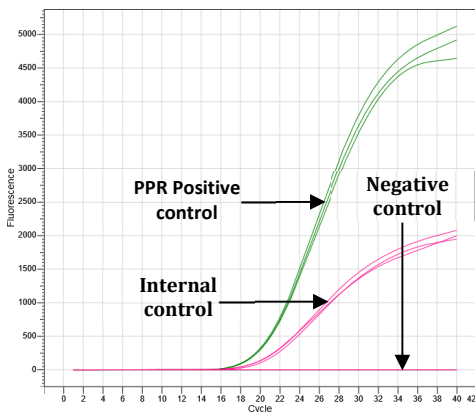

Sr. No.	Sample	Ct value
1.	PPR Positive control	20.99
2.	Internal Control	21.02

Image representing probe based real-time amplification data of PPR with Ct values (provided in table)

### Data Interpretation

Detection channel		Result Interpretation
FAM (PPR)	JOE (Internal Control)	
+	+	Positive for PPR
-	+	Negative for PPR
-	-	PCR inhibition or reagent failure. Repeat PCR or repeat extraction from original sample

Ct value	Result
≤ 35	Detected (+)
> 35 or N/A	Not detected (-)

### Warning and Precautions

Not for Medicinal Use. Read the procedure carefully before beginning the protocol. Wear protective gloves/protective clothing/eye protection/face protection. Follow good clinical laboratory practices while handling clinical samples. Standard precautions should be followed as per established guidelines. Safety guidelines may be referred in safety data sheets of the product.

### Limitations

Although rare, mutations within the highly conserved regions of the targets genes covered by the kit's primers and/or probe may result in under quantitation or failure to detect the presence of the target regions in these cases. Validity and performance of the assay design are revised at regular intervals.

### Quality Control

Each lot of Hi-PCR® Peste des petits ruminants (PPR) Probe PCR Kit is assayed for contaminating endonuclease, exonuclease and non-specific DNase activities. Functionally tested in DNA amplification.

### Performance and Evaluation

Each lot of Hi-PCR® Peste des petits ruminants (PPR) Probe PCR Kit is tested against predetermined specifications to ensure consistent product quality.

### Troubleshooting Guide

Sr. No.	Problem	Cause	Solution
1.	No amplification	Degraded samples	1. Check the integrity of RNA using agarose gel electrophoresis. 2. Use freshly prepared RNA to ensure the availability of intact template sequence for efficient amplification.
		Error in protocol setup	Verify that the correct reagent volumes, dilutions and storage conditions have been used.
2.	Variability between replicates	Error in reaction set-up	Prepare a large volume master mix, vortex thoroughly and aliquot into reaction tubes.
		Air bubbles in reaction mix	Briefly centrifuge reaction samples/plate prior to running on a real-time PCR instrument.
		Pipetting error	C <sub>t</sub> values of replicates can show increased variation due to poor laboratory technique or imprecise pipettes.

3.	Amplification in negative control	Reagents contaminated	1. Replace all critical solutions. 2. Repeat the analysis of all tests with fresh aliquots of critical reagents.
4.	No signal with positive controls	Incorrect programming of the temperature profile of the thermocycler	Compare the temperature profile to the manual.

### Safety Information


HiMedia's Hi-PCR® Peste des petits ruminants (PPR) Probe PCR Kit is for laboratory use only, not for drug, household or other uses. Take appropriate laboratory safety measures and wear gloves when handling.

### Disposal

User must ensure safe disposal by autoclaving and/or incineration of used or unusable preparations of this product. Follow established laboratory procedures in disposing of infectious materials and material that comes into contact with clinical sample must be decontaminated and disposed of in accordance with current laboratory techniques.

### Technical Assistance

At HiMedia, we pride ourselves on the quality and availability of our technical support. For any kind of technical assistance, mail at [mb@himedialabs.com](mailto:mb@himedialabs.com).



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Private Limited,  
Reg. Off: Plot No. C-40, Road No. 21Y,  
MIDC, Wagle Industrial Estate, Thane,  
(West) 400604, Maharashtra, INDIA.  
Web: [www.himedialabs.com](http://www.himedialabs.com)



02/2027

PIMBPCR168\_O/0224

MBPCR168-11

### Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal or therapeutic use but for laboratory, diagnostic, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.